



Centre for Biopharmaceutical Excellence


Microbiology Controls Environmental Monitoring Programs

© CBE Pty Ltd





This training program is copyright to CBE Pty Ltd and may not be modified, reproduced, sold, loaned, hired or traded in any form without its the express written permission.

© CBE – 023 V3

1



Module Topics

-  Fundamental EM Program – what to monitor
-  Frequency, Location and Methods
-  Monitoring Water Systems
-  Managing an EM program for Sterile Cleanrooms

© CBE – 023 V3

Introduction

Some Important References

- EU/PICs/TGA cGMP Annex 1 – Sterile Products
- PDA Technical Report #13 Fundamentals of an Environmental Monitoring Program
- USP <1116> Microbiological Evaluation of Cleanrooms
- FDA Guidance – Aseptic Processing
- ISO 14644 Series - Cleanrooms and associated controlled environments

How Important is Environmental Monitoring ?

- The answer lies in risk assessment
- The GMPs for sterile products has clearly defined GMP rules
- The GMPs for non-sterile products have poorly or un-defined expectations
- How important - depends entirely on:
 - the dose form and use of the product
 - the types of product manufactured (sterile / non-sterile)
 - Whether potent materials are handled in the facility
 - Whether processing is closed or open

WHO Guidance
Environmental Monitoring of Clean Rooms in Vaccine Facilities
Points to consider for manufacturers of human vaccines

- EM describes the microbiological testing undertaken in order to detect changing trends of microbial counts and micro-flora growth within clean rooms or controlled environments.
- The results obtained provide information about the physical construction of the room, the performance of the Heating, Ventilation, and Air-Conditioning (HVAC) system, personnel cleanliness, gowning practices, the equipment, and cleaning operations.
- Use Risk Assessment based on “**Open**” and “**Closed**” systems and considering “**Live**” and “**Inactivated**” materials

Closed vs Open Systems

Closed: Systems are considered closed when materials are added and removed so that product is not exposed to the room environment at any time.

To do so they must be equipped with a barrier technologies allowing the aseptic transfer of solids, liquids, and gasses, such as tube welders, steam-through valves, isolator port assemblies, and other validated transfer systems.

Open: Semi closed or intermittently closed systems for the purpose of defining clean room grades are considered open systems.

Why do we monitor ?

- **Particulates:** Verify that the HVAC systems is functioning correctly and rooms are meeting specifications. Particles are associated with physical contamination and indirectly micro-biological contamination.
- **Microbiological:** The purpose of viable environmental monitoring is to:
 - verify the integrity of the cleanroom air and HVAC systems
 - monitor the effectiveness of surface C&S programs
 - monitor operator performance via personnel monitoring.
 - Monitor aseptic process integrity in Grades A and B

What should be monitored ?

Physical

- Particles at rest
- Temperature
- Relative Humidity
- Room Pressures

Biological

- Bacteria
- Yeast and moulds

Pharmaceutical Services

- Water system and in some cases steam
- HVAC
- Pharmaceutical gases

What Methods (Biological) ?

Each method has limitations

Suitable **combination** of:

- Settle plates
- Contact (RODAC) Plates
- Surface Swabs
- Active Air Sampler
- Flush Water (from Equipment)
- Endotoxin for some sterile products equipment

What Sample Locations to Choose ?

- Defined for particulates generally in ISO14644 and cGMP Annex 1
- **Risk based decision** for micro-biological monitoring
- Microbiological driven by the **purpose of sampling**
- Considerations:
 - Proximity to the product
 - Product contact equipment surfaces
 - Whether testing for cleaning verification or product purity

Example Locations – Sterile Suites

Grade A Space

- Generally only at or above working height
- Near open filled containers (air sample)
- Critical surfaces (post filling swab only)
- Obstacles that may create turbulence (air)
- Curtains and machine doors
- Beneath equipment / floor ?
- Post changeover of lines

Grade B Space

- Proximal to air returns
- Door handles (swabs)
- Obstacles that may create turbulence (air)
- Trolleys
- HMI Consoles
- Floor / Walls/Windows
- Pass throughs
- Adjustment tools

Higher Risk Locations in Grade A

- near open filled containers (air sample)
- proximal to air return (air sample)
- floor and door handles (swabs)
- filling nozzle (post filling swab only)
- gloved hand (contact plate)
- obstacles that may create turbulence (air)

Example Locations – Grades C and D

- Post processing product contact equipment cleaning surfaces
- Hardest to clean locations for direct product contact surfaces
- Rooms with open processing – more frequent
- Rooms with “contained” processing – lesser frequency
- Rooms with closed processing – less frequency
- Non-processing rooms – infrequent
- Air locks
- Drains, washbays ?

How Frequently to Monitor ?

- Is a risk based decision which depends on:
 - the dose form being processed (aseptic / terminal)
 - whether the processing is “closed”, “contained” or “open”
- Sterile products / aseptic processing have defined requirements for Grade A, somewhat for Grade B.
- Grade A and B expect some frequent/continuous coverage – settle plate exposure enable this
- Defined for Grade C and D by WHO Guidance
- Need enough samples to conduct trending over a year
- Some fixed locations and some rotational

WHO Recommended Viables Monitoring Frequencies



Table 5. Microorganism *in-operation* (dynamic) routine monitoring frequencies

Classification	Volumetric ⁽²⁾	Settle plate ⁽²⁾	Contact plate	Glove print
Grade A (filling operations) ¹	Once per shift	Once per shift	Once per shift	Once per shift
Grade B	Daily	Daily	Daily	Daily
Grade C	Weekly	Weekly	Weekly	N/A
Grade D	Monthly	Monthly	N/A	N/A
UDAF in B	Once per shift	Once per shift	Once per shift	Once per shift
UDAF in C	Weekly	Weekly	Weekly	Weekly
UDAF in D	Monthly	Monthly	Monthly	N/A

(2) The practice of air sampling at the start, middle, and end of filling operations provides better environmental monitoring and facilitates investigations related to filling batch release. This approach should be part of a general environmental monitoring strategy based on risk analysis and considering the types of activities performed.

Relative Frequency of Monitoring – Rooms for Non-Sterile Facilities



- **Lowest Risk (I)** - low risk rooms – monitor 1 - 2 months
- **Moderate Risk (II)** – medium risk rooms monitor 2 - 4 weeks
- **Higher Risk (III)** – higher risk rooms – monitor weekly

Room Activity	Dry Oral Solids	Liquid / Creams
No Product / Materials Exposed	I	I
Processing Equipment Storage	I	II
Packaging Areas	I	II
Open Product Exposed	II	III

Examples of Non-Sterile Limits

Cleaned Equipment Limits (Swabs)

Microbiological Limits for Surfaces Swabs (post clean)	Alert Levels per Swab (25cm ²)	Action Levels per Swab (25cm ²)
Surface not in immediate contact with product (e.g. lid)	> 2 cfu/swab Any mould	≥ 5 cfu / swab > 1 mould
Surface in immediate contact with product (e.g. inside tank)	Any positive	≥ 2 cfu / swab Any mould

Cleaned Facility Limits (Air Sample)

Alert Limit			Action Limit		
<i>Bacteria</i>	<i>Yeast Mold</i>	<i>Total Count</i>	<i>Bacteria</i>	<i>Yeast Mold</i>	<i>Total Count</i>
> 25	> 15	> 40	> 50	> 30	> 100

The Paperwork

- Sample Location
- Date sample taken (length of time for settle plates)
- Batch number and expiry of the media
- Operator(s) who took the samples
- State of the room (at rest or in operation and activity)
- Incubation conditions
- Operator reading the plates and date read
- Number of cfu per sample – separate for Yeast / Mold
- Any identification
- Signature of person reviewing the results

Physical Monitoring

Pressure Differentials

- Generally continuous by a validated EMS or
- Magnehelic gauges outside each processing room read twice daily
- Generally > 15Pa (sterile) and > 10Pa (non- sterile) differentials
- Verify air flow directions between rooms “at rest”

Temperature / RH %

- Either EMS system or in- room physical monitors
- Record Max and Min per day

Filter Integrity

- Annual clean and test for % penetration
- Velocity not usually measured for non-sterile rooms, except for validation purposes / air change rate calculations.

WHO Particulate Monitoring

Table 2. Maximum permitted airborne particulate concentration per air grade²

Grade	At rest		In operation	
	Max. permitted particles / m ³		Max. permitted particles / m ³	
	≥ 0.5 µm	≥ 5.0 µm	≥ 0.5 µm	≥ 5.0 µm
A	3,520	20	3,520	20
B	3,520	29	352,000	2,900
C	352,000	2,900	3,520,000	29,000
D	3,520,000	29,000	Not defined	Not defined

Table 3. Monitoring frequencies for *in operation* routine particulate sampling

Classification	In operation (dynamic) routine particulate sampling
Grade A (filling operation)	For the full duration of operation
Grade B	Daily ⁽¹⁾
Grade C	Weekly
Grade D	Not required
UDAF work stations in B	Daily ⁽¹⁾
UDAF work stations in C	Weekly
UDAF work stations in D	Monthly
UDAF in UNC areas	Routine re-qualification of UDAF is sufficient

⁽¹⁾ Working days. Monitoring can be omitted on e.g., weekends if no production activities are taking place.


Pharmaceutical Waters

- Feed (Potable) Water
- Purified Water
- Highly Purified Water
- Water for Injections – PFW & WFI
- Softened Water
- Water for Final Rinse
- Pure, or clean Steam
- Water for cooling Autoclaves

- Each has a different monitoring requirement

What goes on inside your water system if it's not maintained

- Free swimming aquatic bacteria – mostly G-ve .. see this as general background bacterial count
- Biofilm build up on surfaces – see this as intermittent spikes
- Key is a good simple design + periodic validated sanitation strategy

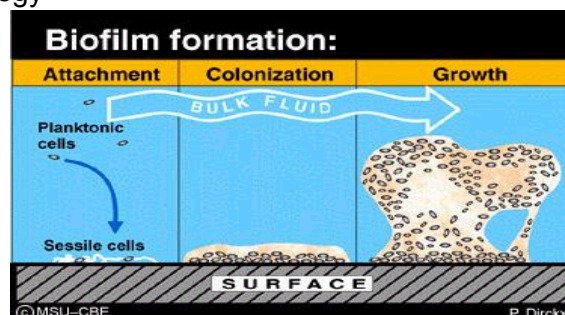

General Water EM Rules

- **Purified water** may use pour plate method:
 - Minimum sample size: 1ml
 - Media: PCA or R2A (depending on limits applied)
 - Incubation: 48 - 72 hours at 30-35⁰C
- **WFI - use membrane filtration:**
 - Minimum sample size: 100ml (use 250mL)
 - Media: R2A agar (low nutrient)
 - Incubation: 48 - 72 hours at 30-35⁰C
 - Monitor endotoxin levels (< 0.25EU/mL)
- Identify recovered organisms to genus level or for WFI to species level.

Water Sampling

- Must have a water system map – with numbered sampling valves for up stream and points of use (POU)
- Pre-clean outlet with 70% alcohol. (TOC sample last.)
- Use “aseptic” technique – requires an SOP
- Sample through production use hoses and flush prior to sampling
- Store samples in fridge unless testing within 4 hours.
Test ASAP (<24 hours)

Water Standards

- British and European Pharmacopoeia monographs
- United States Pharmacopoeia <1231>
- CPMP/QWP/158/01 – Guidance – Quality of water for pharmaceutical use

Microbial Limits - USP <1231>

Manufacturers should establish “**alert**” and “**action**” limits based on the use of the water plus capability of the system. They may involve levels of total microbial counts or recoveries of specific microorganisms

There are certain maximum microbial levels above which action levels should never be established.

Generally considered **maximum action levels** are:

- **100 cfu per mL for Purified Water**
- **10 cfu per 100 mL for Water for Injection**
- **For WFI - LAL < 0.25EU/mL**

CBE
Center for Bioprocess Excellence

Expected Limits

Purified Water	<ul style="list-style-type: none">• Target < 1cfu/mL on average• Alert > 10cfu/mL• Action** >100cfu/mL
WFI	<ul style="list-style-type: none">• Target < 1cfu/100mL “effectively sterile”• Alert > 1cfu/100mL/ any LAL count• Action** > 10cfu/100mL / 0.25 EU/mL

** Should set action limits below compendial limits if possible

© CBE – 023 V3 27

CBE
Center for Bioprocess Excellence

Developing and Managing a Cleanroom Microbiological Monitoring Program for Sterile Products

© CBE – 023 V3 28

Who Should Monitor ?

Oversight by QC Microbiology


QC Led Team

- Independent of Production
- Policeman approach
- Not efficient utilisation of resources

Production Led Team

- Pragmatic approach
- In-process control
- Must have strong QC oversight
 - Training of operators
 - QC surveillance program
 - Random audits by QC

Core EM Documentation

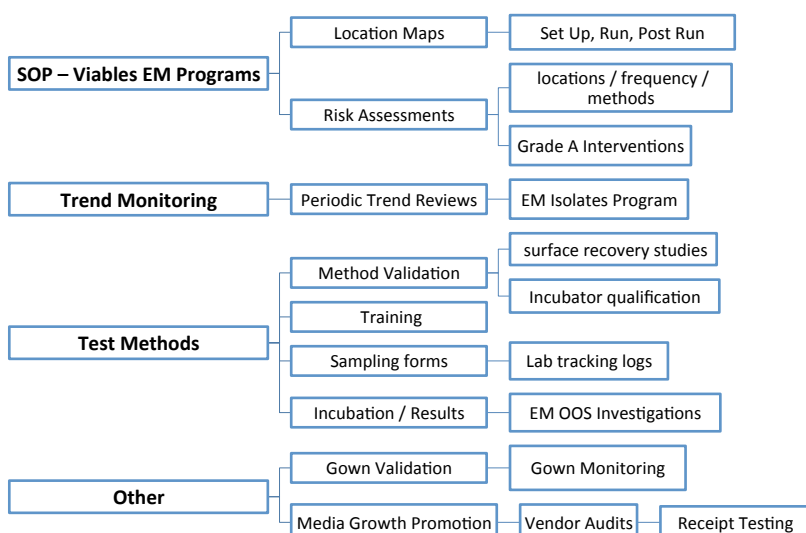

Physical Environment and Airflow Patterns



- Airflow patterns are studied (visualization studies) to:
 - Look for lack of turbulence and no entrainment across Grade B to A interfaces;
 - Identify worst case locations for EM sampling sites
- Must do under “at rest” and simulated “in operation” modes
- Airflow patterns are established during qualification and re-validation studies to ensure the validated conditions have not changed;
 - Grade B to A interfaces
 - Movement through pass through cabinets (PTCs)
- The patterns should be documented so changes can be detected. Require a protocol and report + raw data (video)

GMP Rules for Grade A and B Air Monitoring



- **Non-viable Particles (NVPs)**
 - Grade A must be continuous monitoring during set up and operation
 - Grade B continuous not mandatory, but preferred
 - Must have an SOP for excursion and line clearance
 - There is an “association” between NVPs and microbes
- **Viable Particles (VPs)**
 - Variety of techniques – all have reasons and challenges
 - Settle plates (passive), contact plates, active air, surface swabs
 - Must be continuous monitoring in Grade A and Grade B
 - Must monitor operator gloves, post intervention and on exit of room and gowns periodically
 - Must have alert and action response program

EM Programs and Sanitation

- EM data monitors the effectiveness of the C&S program
- There is no one magic sanitant so a combination is needed.
Vegetative cells → Fungal spores → Bacterial spores
Sanitisers Disinfectants Sporicides.....
- EM Trend reviews underpin confidence in C & S program and cleanroom management
- Should identify & trend fungi/mold separately to bacteria
- For new sanitant should validate effectiveness “in field”.
Sanitant surface residues can inhibit EM growth

Establishing a Viables EM Program for Grade A and B

1. Engage Microbiologist and Aseptic Operators
2. Study the fill line, process, critical space and Grade B Rooms
3. Study personnel and materials movement
4. Conduct air visualisation studies “at rest” then in “simulated operation”
5. Characterisation study for extended period (if possible) grid rooms
6. Risk assess worst case locations:
 - Critical space and critical surfaces
 - Areas with high activity or personnel frequently in proximity
 - Areas with high personnel traffic or areas frequently touched
 - Areas difficult to sanitise effectively
7. 3 times OQ at rest after C&S program
8. 3 times PQ in operation after C&S program
9. SOP - Fixed and rotational locations in 1st 12 months – review 3 monthly then update after review.

Site Selection Considerations

- Can use a combination of grid mapping by room and risk assessment by location in room
 - Sites or process steps where contamination may adversely effect product
 - Sites likely to accumulate microbial load during processing or use
 - Potential “dead spots” in room
 - Sites most difficult to clean or sanitise
 - Means of microbial dispersion in the room environment via:
 - People, equipment, processes, materials and air flows
- Must also consider risk to product associated with the sampling itself
- Must be able to remove any media residue from surfaces
- Must not interfere with operators during processing

Interpreting Viable Industry Limits (Grade A and B Space)

	Active Air cfu per m ³	Passive Air (Settle – 4 hr)	Surface (Rodac/Swab)	Personal (Glove 5 finger)	Personal (Gown)
EU/PICs/Who Annex 1	A < 1 B 10	A < 1 B 5	A < 1 B 5	A < 1 B 5	Not specified
US FDA Class 100	1	1	Not specified	Not specified	Not specified
Class 10,000	10	5			
USP <1116> (incident rate)	ISO 5 <1% ISO 7 <5%	Same incident rate as active air	Same incident rate as active air	Same incident rate as active air	Same incident rate as active air
Japan Aseptic Guide (JPXV1)	A < 1 B 10	A < 1 B 5	A < 1 B 5	A < 1 B 5	Not specified

Interpreting Viable Industry Limits (Grade C and D Space)




	Active Air cfu per m ³	Passive Air (Settle – 4 hr)	Surface (Rodac/Swab)	Personal (Glove 5 finger)	Personal (Gown)
EU/PICs/Who Annex 1	C 100 D 200	C 50 D 100	C 25 D 50	Not specified	Not specified
US FDA Class 100,000	100	50	Not specified	Not specified	Not specified
USP <1116> (incident rate)	ISO 8 <10%	Same incident rate as active air	Same incident rate as active air	Same incident rate as active air	Same incident rate as active air
Japan Aseptic Guide (JPXV1)	C 100 D 200	C 50 D 100	C 25 D 50	Not specified	Not specified


© CBE – 023 V3

37

Grade B Profile

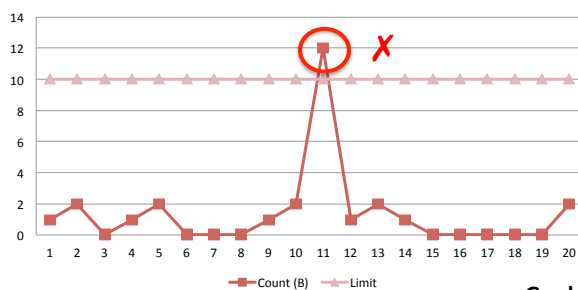

Grade B Profile

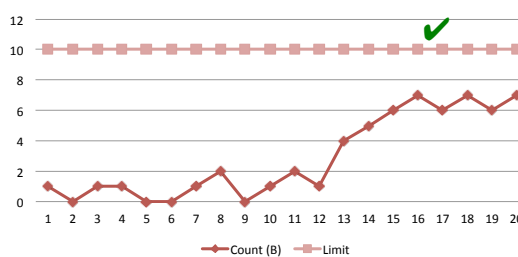

© CBE – 023 V3

38

Minefields in Limit Interpretation

- Numbers matter but trend changes matter as much
- PICs says “on average” but single excursions matter
- Based on total counts but species matter e.g yeast/mold, pseudomads
- Limits have caveats regarding methods / conditions
- Grades B, C and D limits are generally excessive in a well controlled cleanroom
- These are regulatory or “action” limits – companies expected to develop “alert” levels
- USP <1116> proposes incident rates instead of numbers – basis is trend monitoring.
- Significance is related to the proximity to open product

Analysis of Microbiological Data (Modular or Product Specific)

- Cleanroom Environmental Monitoring (Modular)
- Bioburden (can be both product and modular)
- Water Systems (Modular)
- Steam and Compressed Air Systems (Modular)


- Cannot assume “normal” distribution of data
- Most values tend to be “0” – hard to mathematically treat
- Must use other techniques
 - Log e or 10 conversion approach
 - Rank Percentile approach

Analysis of Microbiological Data (Objective)



- Want to verify or re-establish **alert and action limits** based on historical trends.
- Science based approach:
 - Convert to Log10 or Log e – this tends to normalise data = problem of zeros.
 - **Rank in order and cut off at say 95% (action) and 90% (alert)****
 - Use cumulative frequency approach

** minimal mathematics needed

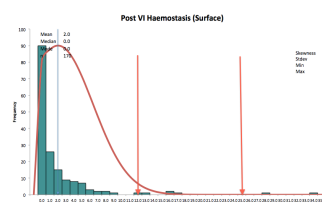

© CBE – 023 V3

41

Using Recovery / Contamination and Incident Rates (Refer to USP – 1116)



Recovery (Contamination) Rate: Number of samples with positive results expressed as a percentage of total samples

Incident Rate: Number of samples with results above the alert / action limits expressed as a percentage of total samples

Manufacturing Facility	Grade C		Grade D	
	Air	Surface	Air	Surface
Number of Samples	237	589	150	409
Number of Samples with growth	95	354	126	253
Recovery Rate	40.1%	60.1%	84%	61.9%
USP <1116> recommendations for recovery	< 5%	< 5%	< 10%	< 10%
Limits (Alert / Action)	50/100	12/25	100/200	25/50
Number of OOL Alert Incidents	2	33	0	12
Number of OOL Action Incident	1	9	4	18
Incident Rate: Alert	0.8%	5.6%	0 %	2.9%
Incident Rate: Action	0.4%	1.5%	2.7%	4.4%
Incident Rate: Total	1.2%	7.1%	2.7%	7.3%

© CBE – 023 V3

42

Alert and Action Limits (based on)



- Risk assessment for new production lines
- Historical trends for established process lines
- Compendial and regulatory guidelines - sterile
 - USP General Information Chapter<1116> Microbiological Evaluation of Clean Rooms and Other Controlled Environments
 - EU-GMP Annex I Manufacture of Sterile Medicinal Products
- All monitoring results should be reviewed regularly to detect trends and to confirm the effectiveness of the cleaning and sanitation program
- Generally QA/QC review: monthly, quarterly and as part of annual review program.

Example Setting Action and Alert Levels Using Ranking



cfu count	Rank	Percent	
59	1	100.0%	
33	2	97.9%	Action @ 95%
22	3	95.9%	
18	4	93.8%	Alert @ 90%
18	5	91.8%	
18	6	89.7%	
17	7	87.7%	
16	8	85.7%	
14	9	83.6%	
12	10	81.6%	
11	11	79.5%	
11	12	77.5%	
10	13	75.5%	
10	14	73.4%	
10	15	71.4%	
etc	etc		

Range of approaches used but need to set alert / action limits scientifically;

Ranking cut off is only one approach;

Must have sufficient data available;

Action Limit \leq Regulatory limit;

Exceeding alert limit is not grounds for corrective action;

Rank Percentile Approach to Establishing Alert and Action Limits.

Data1	Point	Data1	Rank	Percent	
30	53	320	1	100.0%	
5	1	30	2	97.2%	99th Percentile
25	49	30	2	97.2%	
15	3	25	4	94.4%	95th Percentile
5	54	25	4	94.4%	
5	10	20	6	93.0%	
15	4	15	7	87.5%	90th Percentile
15	7	15	7	87.5%	
5	8	15	7	87.5%	
20	12	15	7	87.5%	
5	2	5	11	77.7%	
15	5	5	11	77.7%	
5	6	5	11	77.7%	
0	9	5	11	77.7%	
0	11	5	11	77.7%	
0	13	5	11	77.7%	
0	18	5	11	77.7%	
5	14	0	18	0.0%	
0	15	0	18	0.0%	
0	16	0	18	0.0%	
0	17	0	18	0.0%	
0	19	0	18	0.0%	
0	20	0	18	0.0%	

Action Limit

Alert Limit

© CBE – 023 V3

45

Example Alert and Action Responses

If	Then also refer to SOP xxxx
Any result exceeds the alert limit (or there is a trend)	<ul style="list-style-type: none"> Identify the organism to genus level Inspect the cleaning record for the equipment to verify it was properly cleaned and sanitized Notify the QC Manager of the result Initiate Alert Report (F xxxx) to notify the QA Manager and Production Manager
Any result exceeds the action limit	<ul style="list-style-type: none"> Identify the organism to species level Inspect the cleaning record for the equipment to verify it was properly cleaned and sanitized Review the testing trends for all equipment used in non-sterile production Notify the QA Manager of the result – determine whether a product risk assessment is warranted, or not. Test the product for the absence of the identified organism Initiate Deviation Report (F xxx) to notify the QA Manager and Production Manager

© CBE – 023 V3

46

EM Excursions and Product Quality

- *“Alert and action limits do not define product attributes such as sterility and therefore should not be considered as product specifications or extensions of the product specification.”*
- *“Rather they are intended to indicate changes so that corrective action may be taken before product quality is adversely affected.”*
- *“Investigations are expected for action level excursions or adverse trends.” (Using a written investigation plan)*

PDA TR 13 EM Fundamentals 2014

Environmental Monitoring: Relationship to Batch Release

- While an inferential relationship exists between microbiological environmental monitoring data and batch release, reaching or exceeding and action level does not necessarily indicate that product quality is adversely affected.
- The significance of action level excursions in environmental monitoring is based upon the outcome of a comprehensive investigation of all conditions that might impact the acceptability of the process and the batch(es) produced.
- The results of such an action level investigation may indeed lead to the rejection of a batch (e.g., problems at filling line plus action levels in multiple environmental monitoring programs) or may not lead to the rejection of a batch (e.g., isolated event, no action levels in multiple environmental monitoring programs, data acceptable before and after event, similar events in successful media fills).

Example of Good EM Annual Review



Grade	Type of Monitoring	Filling Room # 1	Filling Room # 1 Vial Storage	Filling Room # 2
A	Active Air	561	187	19
	Passive Air	561	187	19
	Surface	1587	0	56
	Total EM Samples	2659	374	94
	Number Positives	0	0	0
B	Active Air	561		38
	Passive Air	0		19
	Surface	2171		220
	Total EM Samples	2732		277
	Number Positives	0		0

© CBE – 023 V3

49

The type of bug matters !



- Mold is a problem in any facility – hard to remove.
 - Set mold limits lower than for total bacterial count limits
- Pseudomonas sp. in water systems and liquids and creams areas
- Known objectionable organisms / pathogens

Should occasionally “speciate” the organisms detected and always when there are unusually high numbers or during an investigation.

© CBE – 023 V3

50

What methods are suitable?

Each method has limitations and advantages so needed in combination.

Suitable **combination** of:

- **Settle plates** – passive limited space but extended time coverage
- **Contact (RODAC) Plates** – small flat surface areas
- **Surface Swabs** – larger inaccessible areas but harder to recover
- **Active Air Sampler** – better detection but limited time duration
- **Gloves and garments monitoring** – hit or miss.

How to Report EM results

- **TAMC** = Total Aerobic Microbial Count
- **TYMC** = Total Yeast and Mold Count
- **TAMC** = TYMC + total bacterial count
- Never report “zero” always NOD (No Organisms Detected)
- **TNTC** = To Numerous To Count (generally means > 300 cfu per plate.)

WHO Recommended Incubation Methods



- Minimum of two temperatures to detect both bacteria and fungi.
- 3 to 5 days of incubation at 20 to 25°C followed by incubation 30 to 35°C for an additional 2-3 days
- The method chosen should be carefully validated and standardized.
- Option for Separate Incubation Conditions:
 - Y & M: 20°C - 25°C for 5 days (SAB or TSA plates) and
 - Bacteria: 30°C - 35°C for 3 days – TSA Plates

EM Test Method Validation - Plates



- Required but limited to % recovery and fertility

EM Settle Plates

- Qualify plates per supplier by recovery study > 70% expected. (WHO recommends > 50%)
 - Add say 100 cfu to the plate then count % recovered for a bacteria, a yeast and a mold
- Consider sanitant inhibitor plates
- 4 hour exposure
- Use near expired plates
- Add back specified organisms, or alternative

EM Test Method Validation - Surface

- Required but limited to % recovery and fertility

EM Swabs

- Add say 100 cfu to cleanroom (representative) different surfaces then count % recovered for a bacteria, a yeast and a mold
- Expect >70% recovery (WHO recommends > 50%)
- Are qualifying each "swabber" technique
- Consider sanitant inhibitor – peptone water

Grade A Critical Space and Critical Surfaces

Critical Space – Grade A / ISO 5

A critical area is one in which the sterilized drug product, containers, and closures are exposed to environmental conditions that must be designed to maintain product sterility.


Critical Surfaces within Critical Space

Not all Grade A space is a critical surface.

Surfaces that may come into contact with or directly affect a sterilized product or its containers or closures.

Critical surfaces are rendered sterile prior to the start of the manufacturing operation, and sterility is maintained throughout processing. Generally monitored post processing.

Critical Space and Critical Surfaces

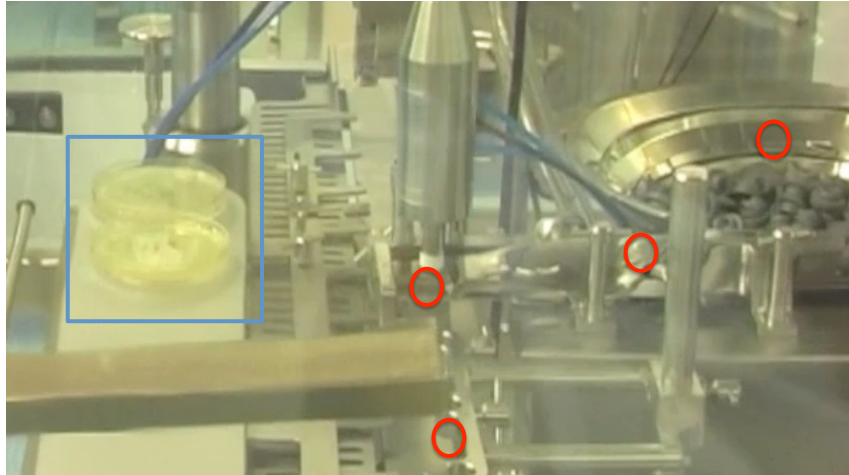

© CBE – 023 V3

57

Personnel Monitoring Aseptic Operators

Sterile Gowns

- Initial qualification 3 times per operator
- 6 or 12 monthly gowning verification
- End of day surveillance - operators in rotation
- Multiple spots in rotation


Gloves

- Initial qualification
- End of aseptic session / end of shift in rotation
- Post entry into Grade A space for all “high risk” interventions
- Left and right hands – 5 fingers

© CBE – 023 V3

58

Gown and Glove Monitoring with Rodacs

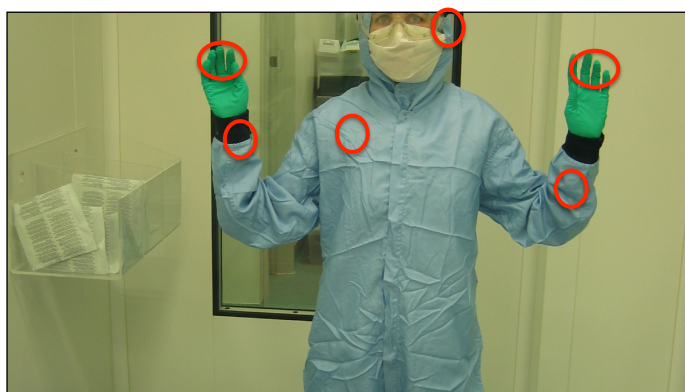

© CBE – 023 V3

59

Grade A / B Excursions and Investigations

- Sample type - contact plate, settle plate, active air sampler, gown)
- Location of sample (distance to critical surfaces)
- Review of relevant air visualisation / smoke studies
- Microbiological identity to species level
- Review of operations during time period (include operator interview, video review, review of event logs)
- Review of relevant EM data (micro, physical - differential pressure, non viables, temp, humidity)
- Review of trend data (historical and after the event)
- Further investigations in regard of potential sample contamination either during sampling or in the labs
- Specific monitoring programs to support root cause investigations

© CBE – 023 V3

60

Crucial information for EM Excursion Risk Assessments

- Is it an isolated event (only 1 sample contaminated)?
- Quantity of contamination (e.g 1 CFU or 25 CFU)
- What is the type of organism ?
- Identification of microorganism (human origin, mold, etc.)
- Plausible most probable root cause(s) informs assessment of product exposure or impact
- Distance to open product and/or critical surface (including airflow pattern)

Usual suspects - sources of organisms

- Personnel ! Operators, cleaners, fitters, transients
- Personnel ! Poor gowning practices
- Personnel ! Poor aseptic techniques / hand sanitisation
- Tracked in via ancillary equipment – trolleys, tanks etc.
- Poor aseptic transfers of materials through pass through etc.
- Inadequate cleaning eg. underneath equipment or on conveyors

Case Example # 1

- Single Grade A organism – *Bacillus. subtilis*
- Contact plate post filling
- Detected on guard rail for vials near filling station
- Track record of line is good
 - No sterility failures
 - No media fill fails
 - Excellent history of EMs in last 2 years
 - Operators are qualified and well trained

Investigation

- Source
- Fate of the batch
- Corrective Action(s)

In summary

- EM is expensive and outcomes can be problematic
- Must pay attention to the small details
- No direct relationship to product quality – degrees of separation is important
- Risk assessment and trend monitoring are fundamental elements
- The more distance between personnel and critical space / surfaces the better case for RABS and Isolator technology.

Some Questions to Discuss



© CBE – 023 V3

Revision

65

Environment Quiz ?

- Should airflow pattern studies be videotaped?
- What are the recommended particulate and microbial alert and action levels for aseptic processing areas?
- Are environmental monitoring alert and action levels considered specifications
- What is the relationship between environmental monitoring and batch release?
- Is continuous viable environmental monitoring required in Grade A (Class 100) areas?

© CBE – 023 V3

Revision

66

Environmental Monitoring Quiz ?

- When and where should air monitoring be conducted for **non-viable particulates** (NVPs)?
- When and where should air monitoring be conducted in aseptic Cleanroom for **viable particulates** (VPs)?
- Should viable monitoring be expected on sterilized product contact surfaces?
- What microbial identification strategy is expected Grade A environmental monitoring samples? Why ?
- Should personnel be monitored when they conduct an interventions ? Why ?



Steve Williams,
 Director, CBE Pty Ltd
www.cbe-ap.com.au
 ☎ +61(0)417116476
 ✉ steve.williams@cbe-ap.com.au

