


Free space superheat to be less than 2°C above control point for rest of cycle.

Free space superheat to be Less than 5°C above control point for first 60 sec.

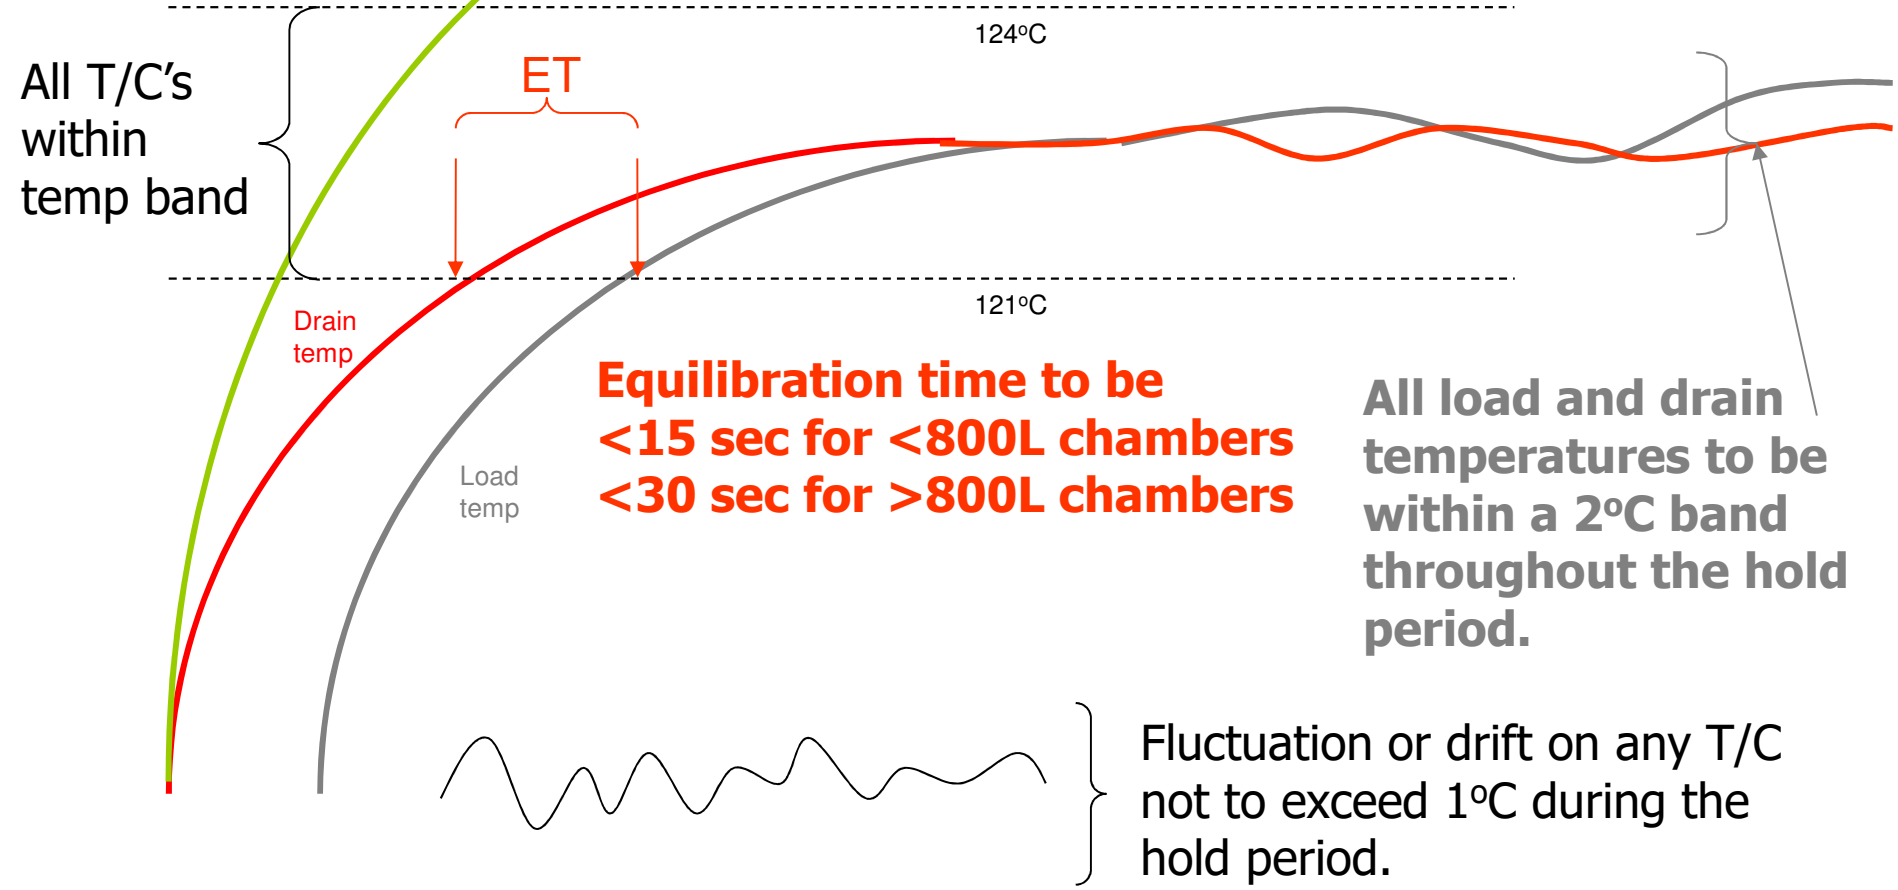

All T/C's within temp band

124°C

ET

Drain temp

121°C

Load temp

Equilibration time to be <15 sec for <800L chambers <30 sec for >800L chambers

All load and drain temperatures to be within a 2°C band throughout the hold period.

Fluctuation or drift on any T/C not to exceed 1°C during the hold period.